


# YOU CAN DO IT

WITHOUT LANCETS\*



## Discover the FreeStyle Libre 2 system



Now available with  
optional glucose alarms

  
**FreeStyle**  
**Libre 2**  
FLASH GLUCOSE MONITORING SYSTEM

  
*life. to the fullest.®*  
**Abbott**


The FreeStyle Libre 2 flash glucose monitoring system is indicated for measuring interstitial fluid glucose levels in people aged 4 years and older with diabetes mellitus. Always read and follow the label/insert.

The FreeStyle Libre 2 app and the FreeStyle Libre 2 reader have similar but not identical features. Finger pricks are required if readings do not match symptoms or expectations. The FreeStyle Libre 2 sensor communicates with the FreeStyle Libre 2 reader that started it or the FreeStyle Libre 2 app that started it. The FreeStyle Libre 2 app is only compatible with certain mobile devices and operating systems. Please check the website for more information about device compatibility before using the app. Use of FreeStyle Libre 2 requires registration with LibreView.

\* Scanning the sensor does not require lancets.

# Experience the freedom of glucose monitoring from your phone

## FreeStyle Libre 2 app

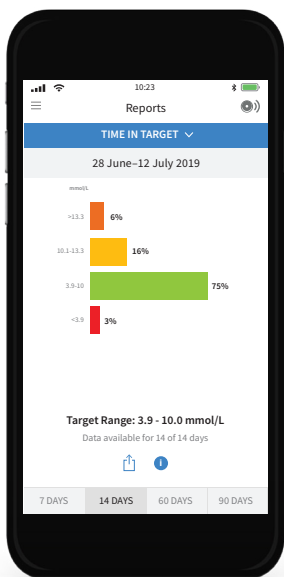

- Get real-time glucose readings on your phone
- Easy-to-read reports showing glucose patterns and trends
- Easily connect and share your glucose information with your healthcare professional

**Download the FREE  
FreeStyle Libre 2 app**

# Free yourself from finger pricks\*

## The FreeStyle Libre 2 system:



### Easy to use<sup>1</sup>

A **painless<sup>2</sup> 1-second scan** shows you your current glucose reading, an 8-hour history, and a trend arrow telling you where your glucose is heading



### Discreet

A small sensor that is **easy to apply** and **comfortable to wear<sup>2</sup>** for up to 14 days

Scan the sensor **discreetly through clothes<sup>†</sup>**



### Reduces A1C

Clinically proven to **significantly lower A1C<sup>3</sup>**



### Optional glucose alarms

Real-time **alarms let you know the minute your glucose is too low or too high**


Data collected with the FreeStyle Libre system: The FreeStyle Libre 2 system has the same features as the FreeStyle Libre system but with optional real-time glucose alarms. Therefore, study data are applicable to both products.

\* Finger pricks are required if readings do not match symptoms or expectations.

† The reader can capture data from the sensor when it is within 1 cm to 4 cm of the sensor.

**References:** 1. Data on file, Abbott Diabetes Care Inc. 2. Haak T, Hanraire H, Ajan R, Hermanns N, Riveline JP, Rayman G. Flash glucose-sensing technology as a replacement for blood glucose monitoring for the management of insulin-treated type 2 diabetes: a multicenter, open-label randomized controlled trial. *Diabetes Ther.* 2017;8(1):55-73. 3. Kröger J, Fasching P, Hanraire H. Three European retrospective real-world chart review studies to determine the effectiveness of flash glucose monitoring on HbA1c in adults with type 2 diabetes. *Diabetes Ther.* 2020;11(1):279-291.

# Get to know your glucose reading

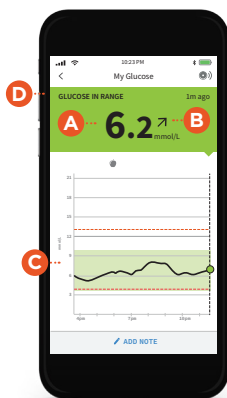

- A Current glucose** provides an accurate glucose reading
- B Glucose trend arrow** shows you where your glucose is heading
- C Glucose graph** shows you an 8-hour history of glucose levels
- D Glucose message** tells you if glucose is in or out of range

**Your scan is more than just a single number at a single point in time. See how small changes to food, medication and activity can change your readings. The more you scan, the better you do.<sup>1-3</sup>**

Data collected with the FreeStyle Libre system. The FreeStyle Libre 2 system has the same features as the FreeStyle Libre system but with optional real-time glucose alarms. Therefore, study data are applicable to both products.

**References:** 1. Lang J, Jangam S, Dunn T, Hayter G. Expanded real-world use reaffirms strong correlation between scanning frequency of flash glucose monitoring and glucose control [Poster 972]. *Diabetes*. 2019;68(suppl 1). 2. Bolinder J, Antuna R, Geelhoed-Duijvestijn P, et al. Novel glucose-sensing technology and hypoglycaemia in type 1 diabetes. *Lancet*. 2016;388(10057):2254-2263. 3. Dunn TC, Xu Y, Hayter G, Aijan RA. Real-world flash glucose monitoring patterns and associations between self-monitoring frequency and glycaemic measures: A European analysis of over 60 million glucose tests. *Diabetes Res Clin Pract*. 2018;137:37-46.



# What would you do with a little more freedom?



Ask your healthcare professional about the FreeStyle Libre 2 system today. For more information, visit **MyFreeStyle.ca**.



© 2021 Abbott. FreeStyle, Libre, and related brand marks are marks of Abbott. Product images are for illustrative purposes only. Other trademarks are the property of their respective owners.

ADC-24763 v2.0